

FIGURE 1

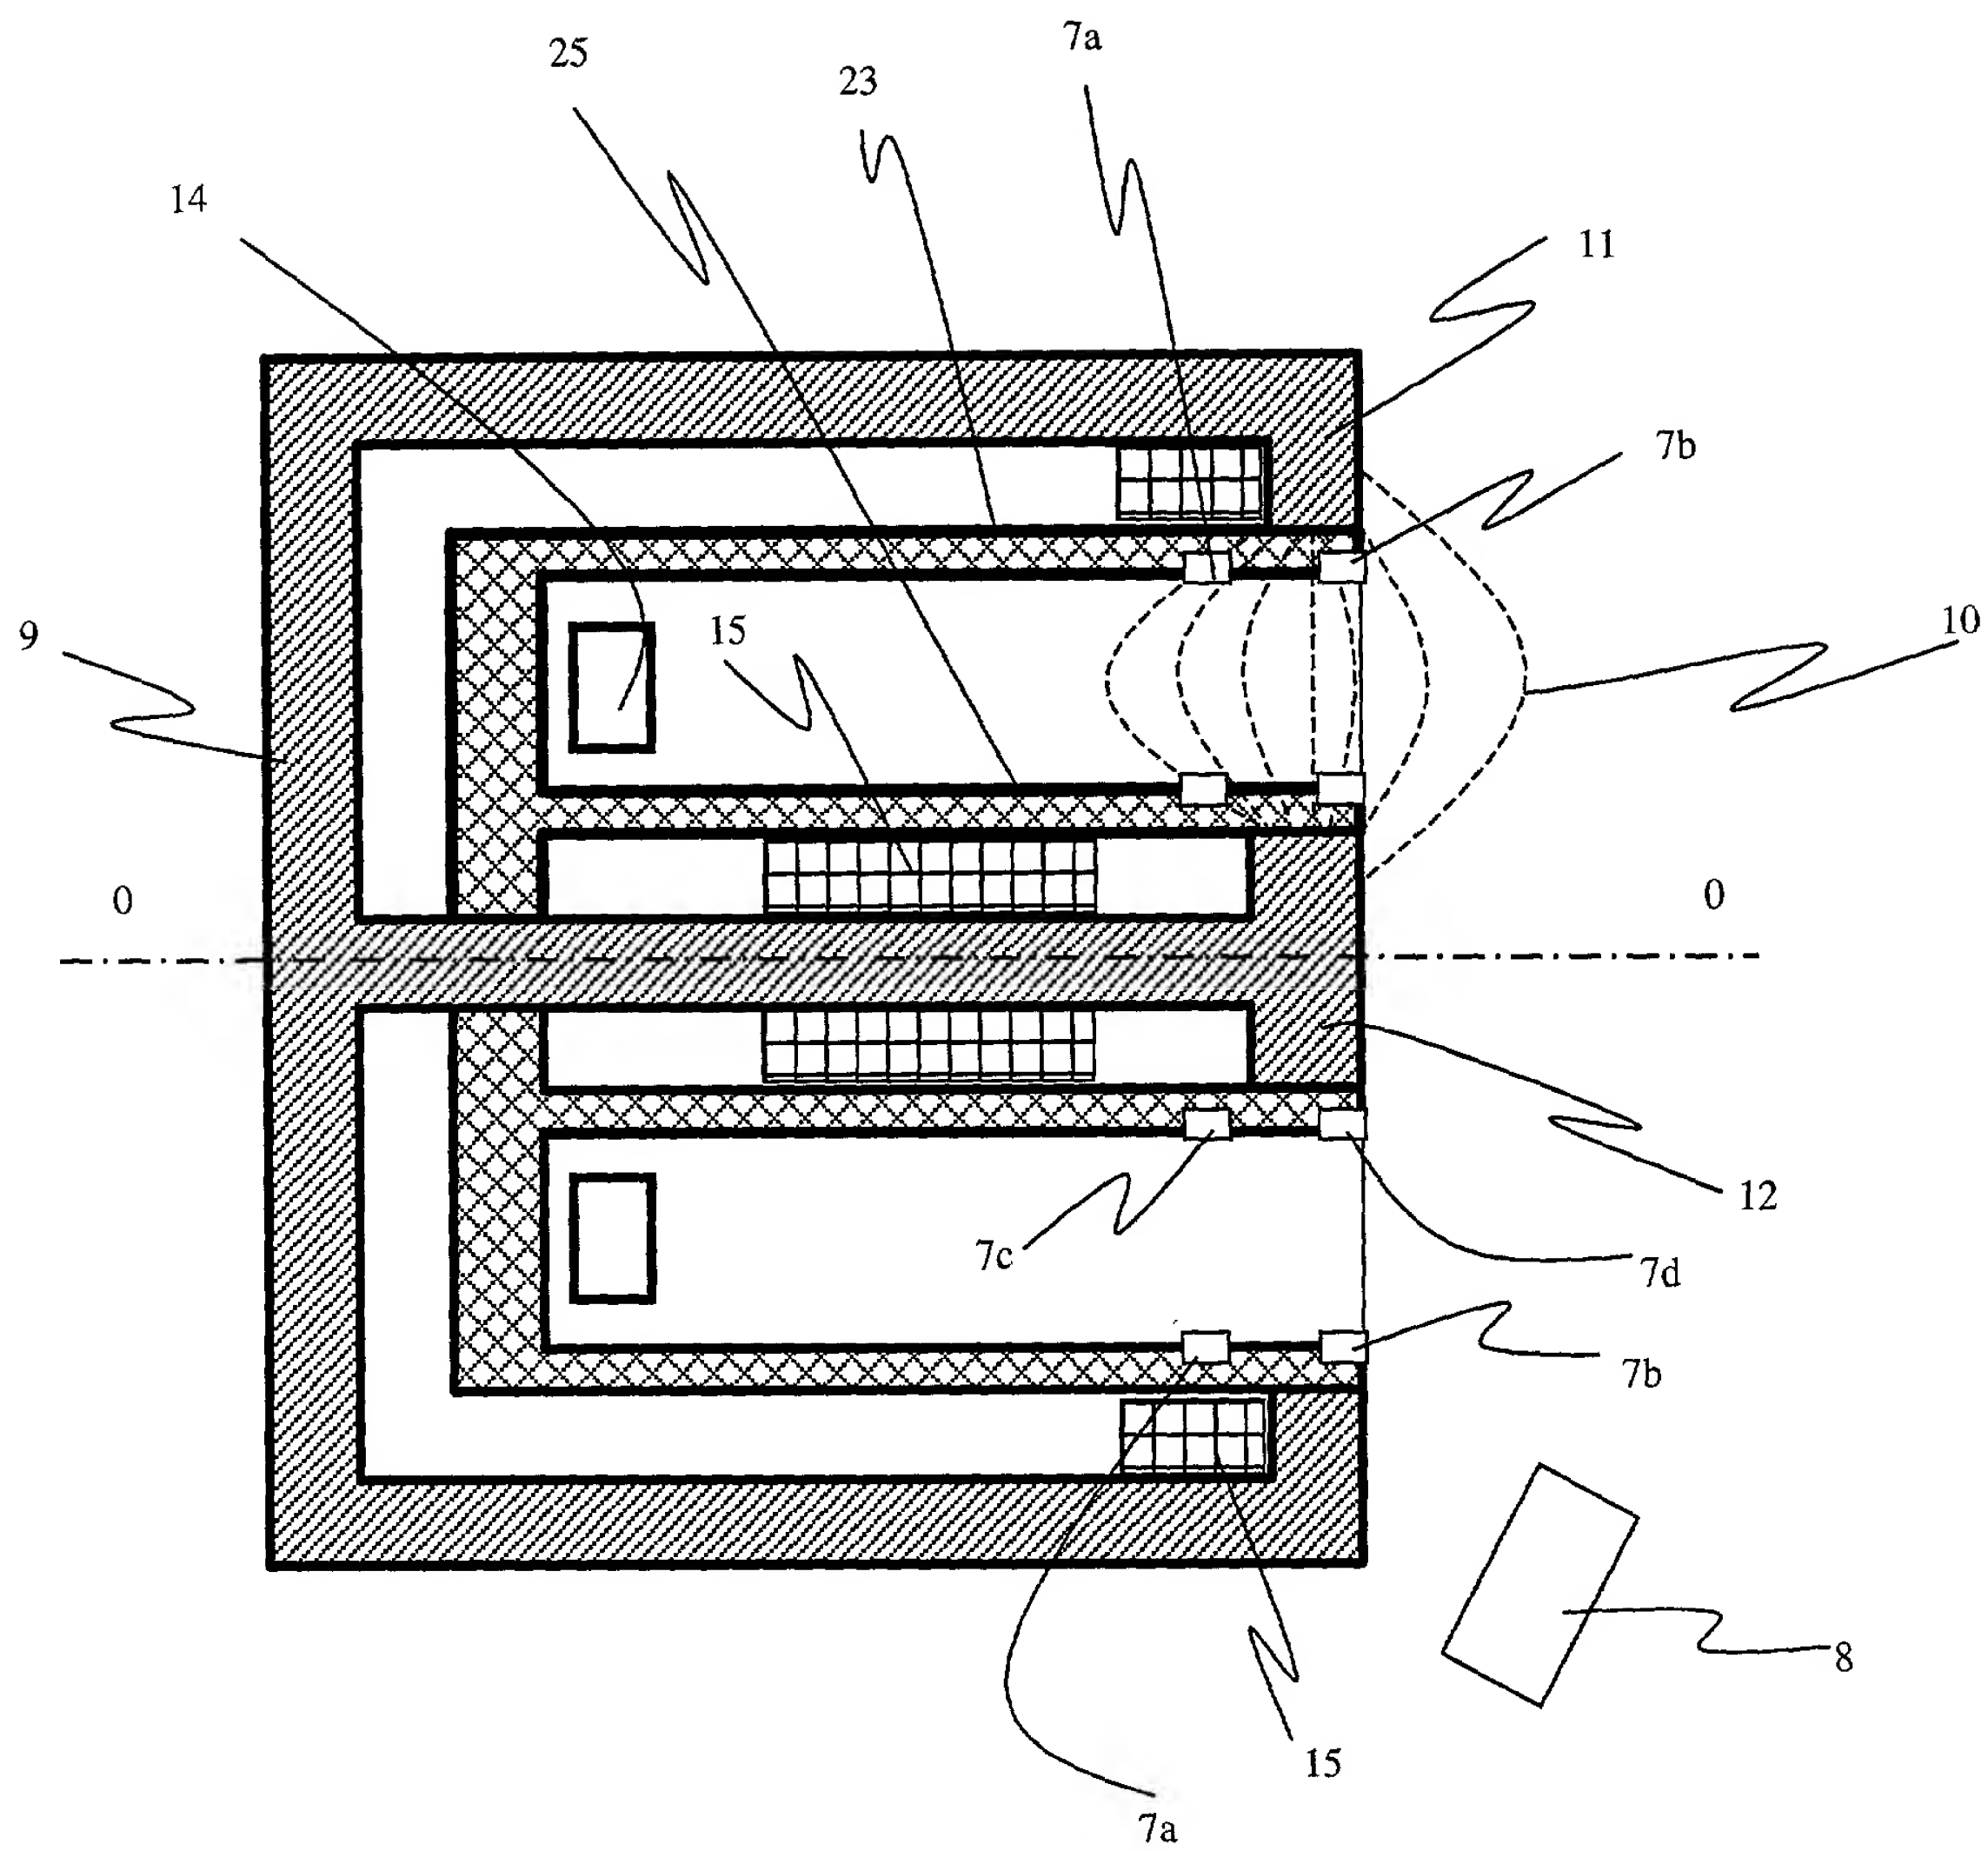


FIGURE 2

FIG. 3 is a cross-sectional view of the device 100 in a closed position.

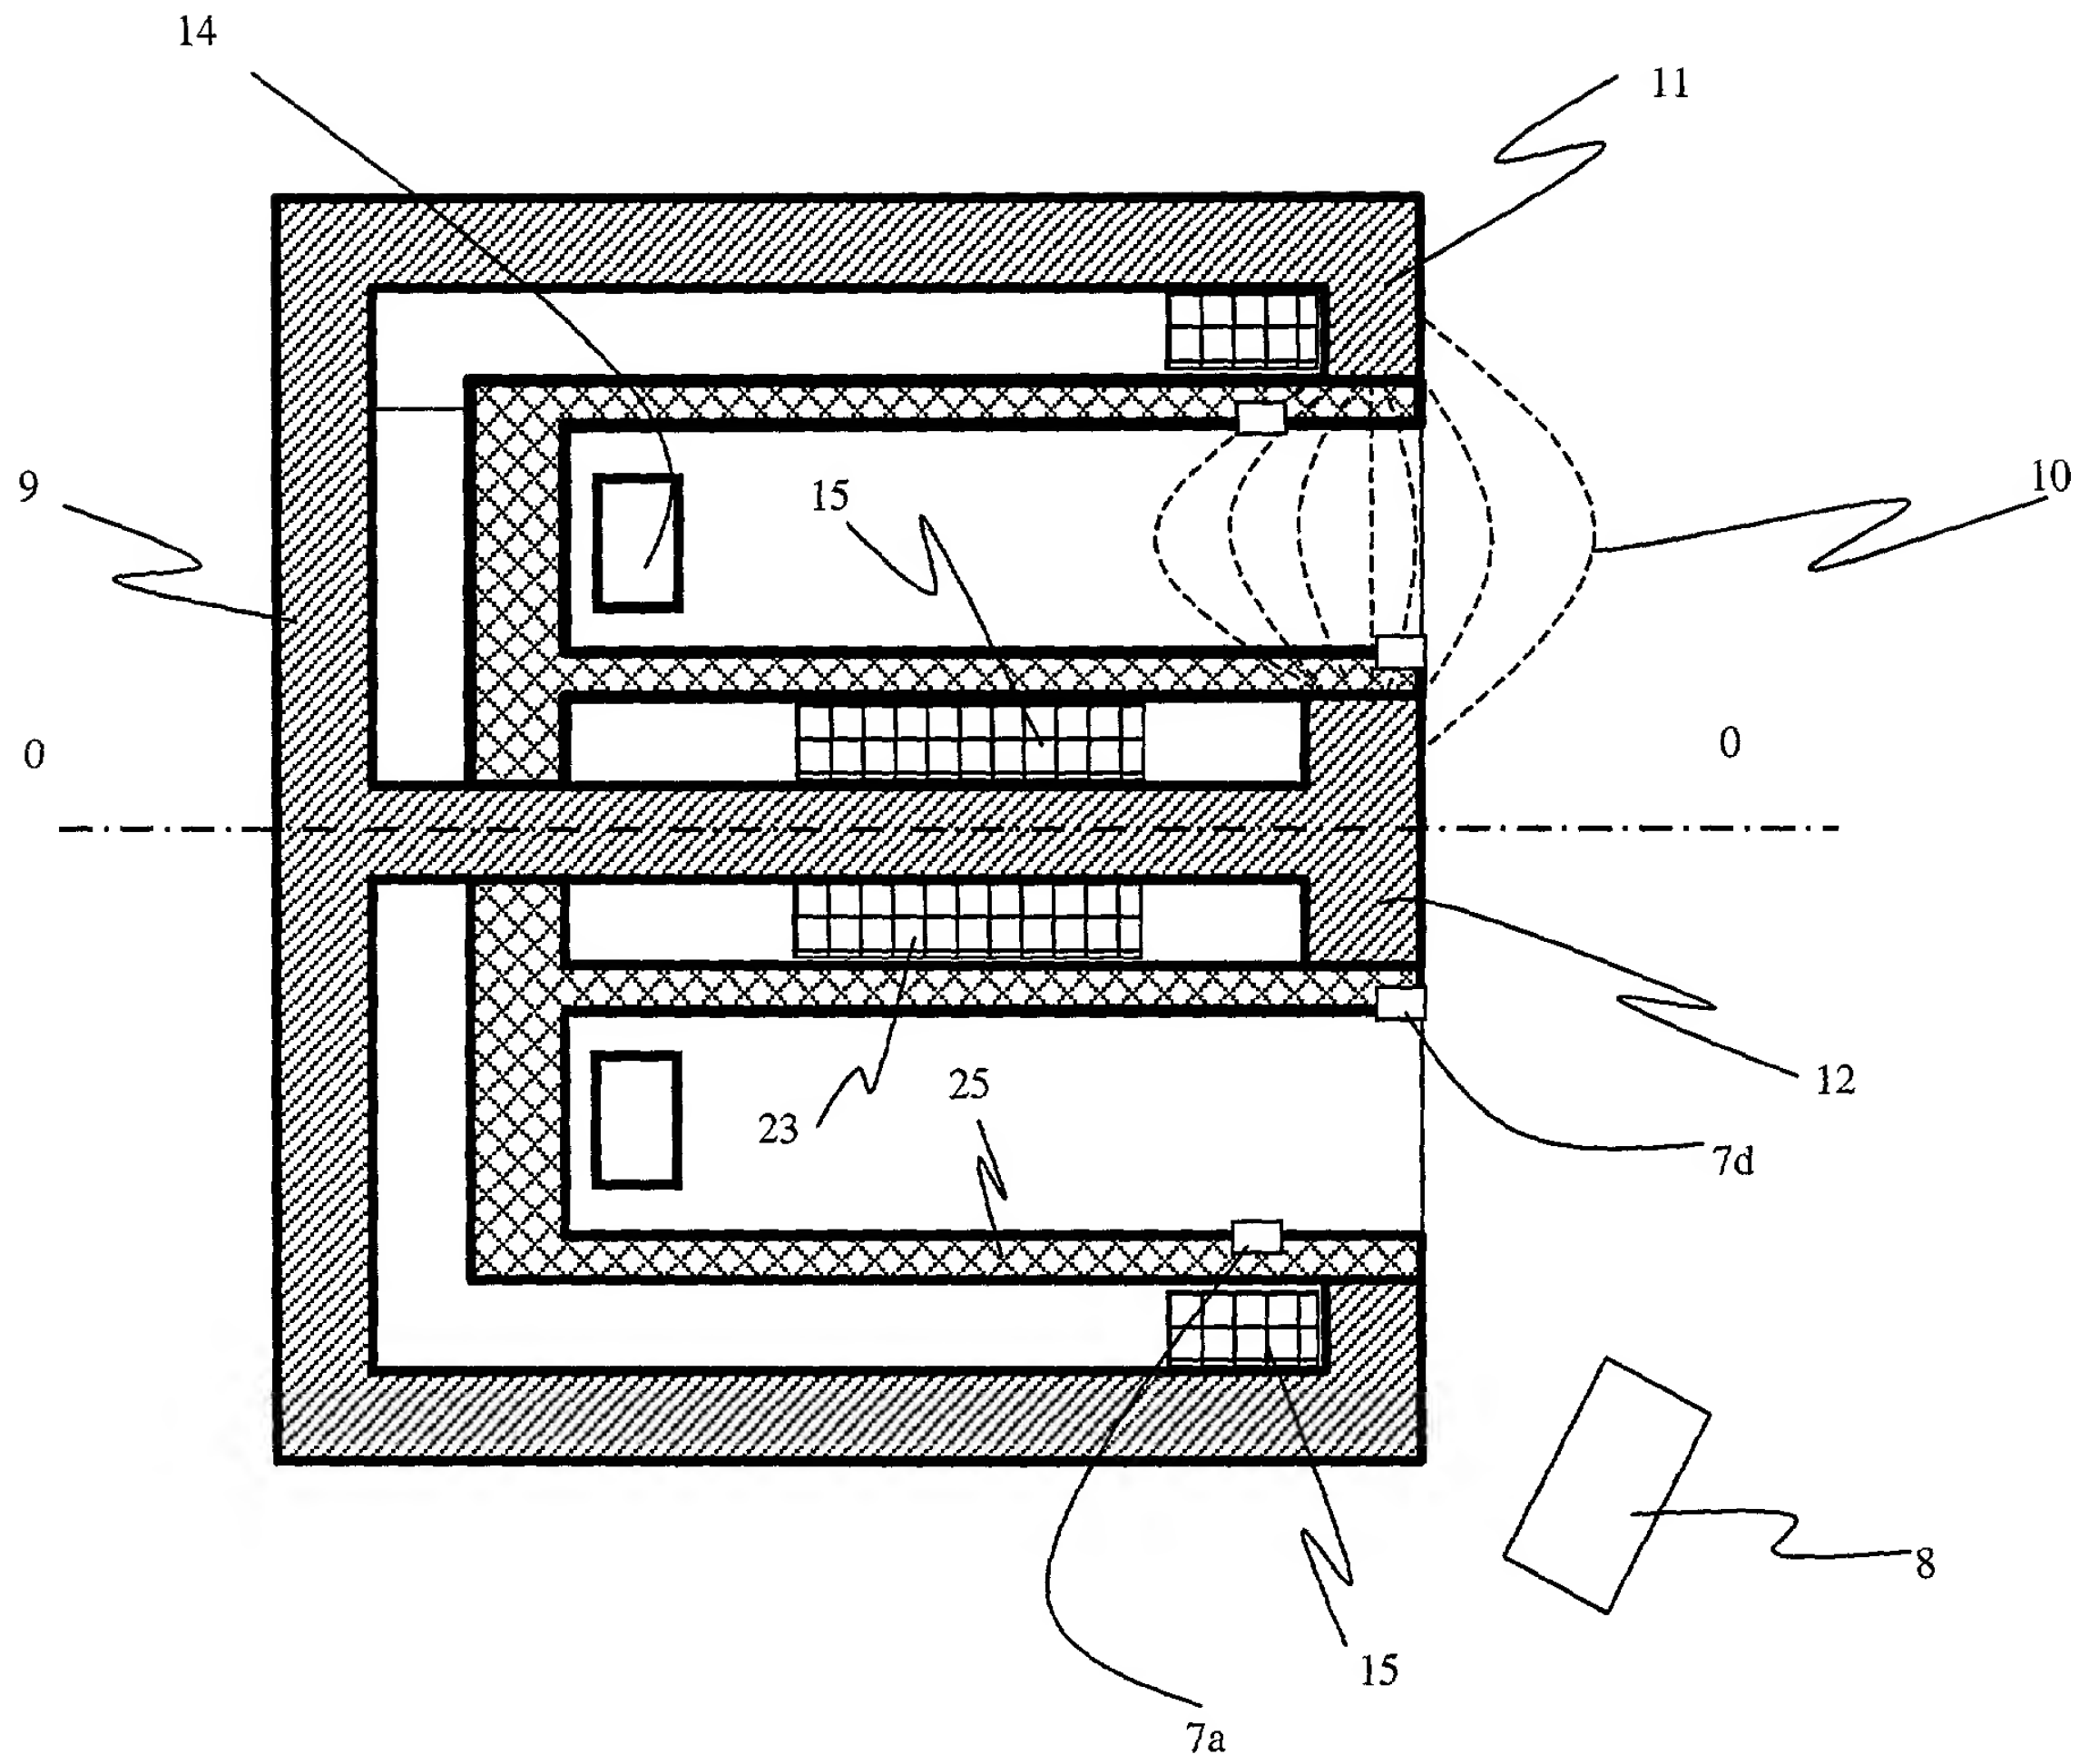


FIGURE 3

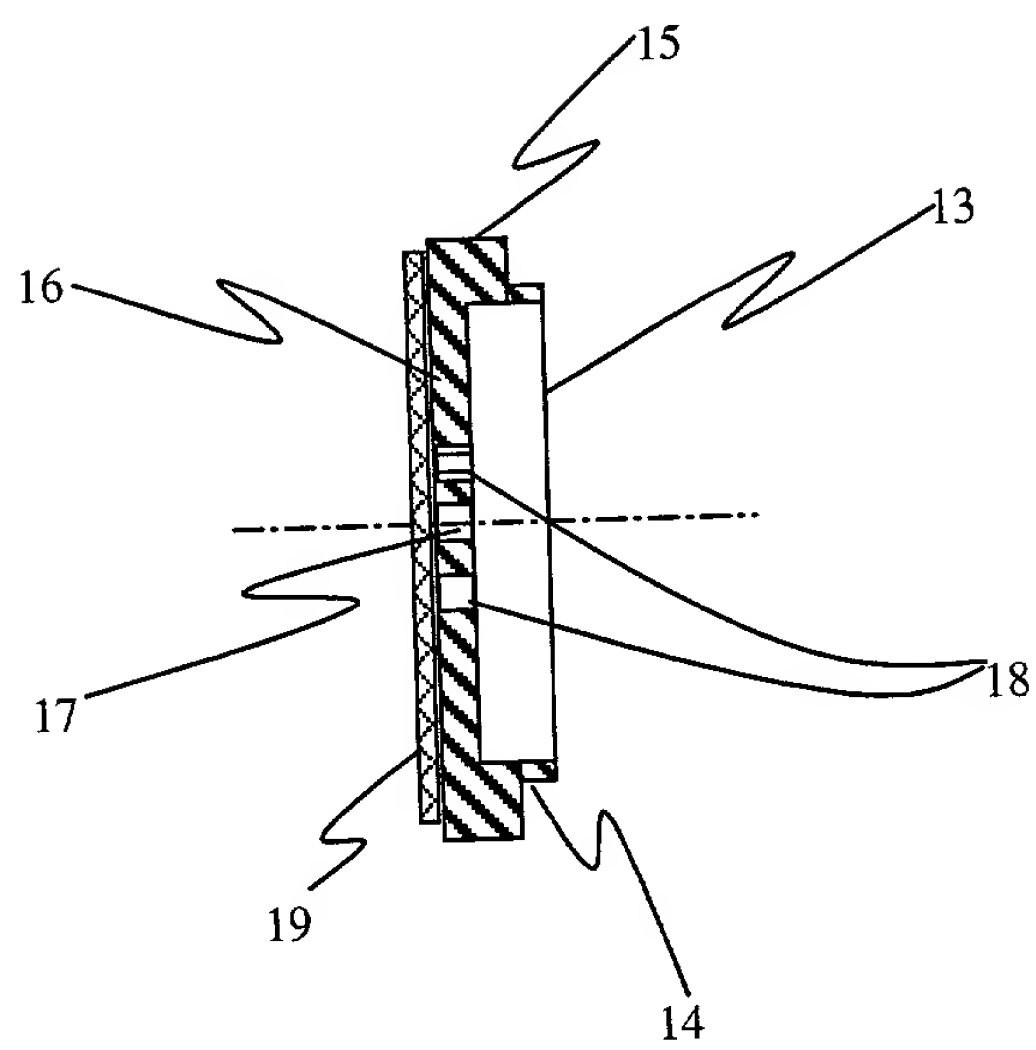


FIGURE 4